

REPORT 2

[2020]

PROJECT TITLE: Detection and Separation of Recyclable Plastics from Municipal Solid Waste (Year 2)

PRINCIPAL INVESTIGATOR(S): Debashis Chanda, PhD, Nanoscience Technology Center, debashis.chanda@ucf.edu, 407-823-4575

PROJECT WEBSITE: <https://www.nanoscience.ucf.edu/research/hinkley-project-2.php>

Work accomplished during this reporting period:

Task 1: Infrared spectrometer device prototype

- The optical benchtop setup from last update was modified and multiple iterations were performed to optimize the alignment of the collected signal as well as the signal-to-noise ratio at the detector.
- The workstation software was further modified to automate the process of scanning the movable mirror while simultaneously measuring the detector signal at different wavelength parameters.

Remote handheld scanner development: In our current work we are developing a stand-alone MIR spectrometer as a testbed for producing deployable solutions to plastic recycling at multiple levels. An infrared light source is reflected off a test sample and the reflected light is gathered into a small collimated beam and passed through a zinc selenide (ZnSe) prism. This prism passes light in the region from 0.6 to 16 microns and spreads this spectrum by wavelength. A rotating mirror scans this spectrum across an infrared detector, thus recording reflected energy vs. wavelength for the plastic sample. The optical system schematic is shown in Figure 1.

This design could be used to produce a fieldable prototype, but it is even more valuable as a starting point, or testbed, to investigate modifications that could be deployed in multiple fieldable implementations. Data gathered on this spectrometer can be used to investigate the specific spectral characteristics necessary for discrimination of plastic types. The following possibilities are examples of the system requirements we will investigate.

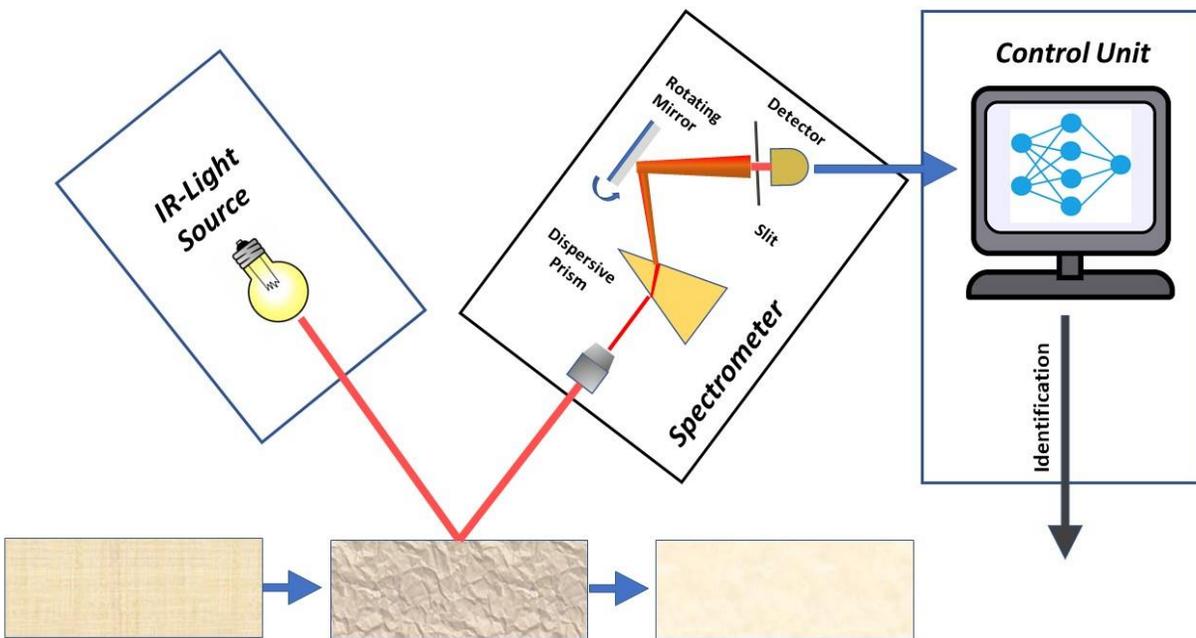


Figure 1. Schematic of the IR optical system showing the light source, the light collection and spectrometer, and the control and data processing modules.

- If the spectral region to be scanned can be limited to a single octave, that is, a factor of 2, then the prism could be replaced by a diffraction grating. Examples of possible octaves would be 3 to 6 microns, 4 to 8 microns, or 6 to 12 microns, each spanning a factor of 2 in wavelength. Use of a diffraction grating rather than a prism simplifies the ultimate design, making it smaller and easier to produce for a handheld device.
- Work last year indicated that 100 data points could be adequate for plastic spectral identification. If the required spectral resolution can be further reduced, to 10 points for example, slit sizes can be increased and spectral dispersion requirements can be relaxed. This would allow a design that is more compact and easier to align, with less attenuation of reflected light signal.
- It is possible that the spectral sampling can be limited to a few, say 4 or 5, specific wavelengths. If this is the case, the design could be modified to use tunable IR lasers or IR LEDs as the light source. This would yield a version of the design especially suited to be deployed to scan large volumes of plastic travelling on conveyor belts.

This spectrometer could be useful in its current configuration as a fieldable solution, but it is hoped it will point the way to even more useful implementations.

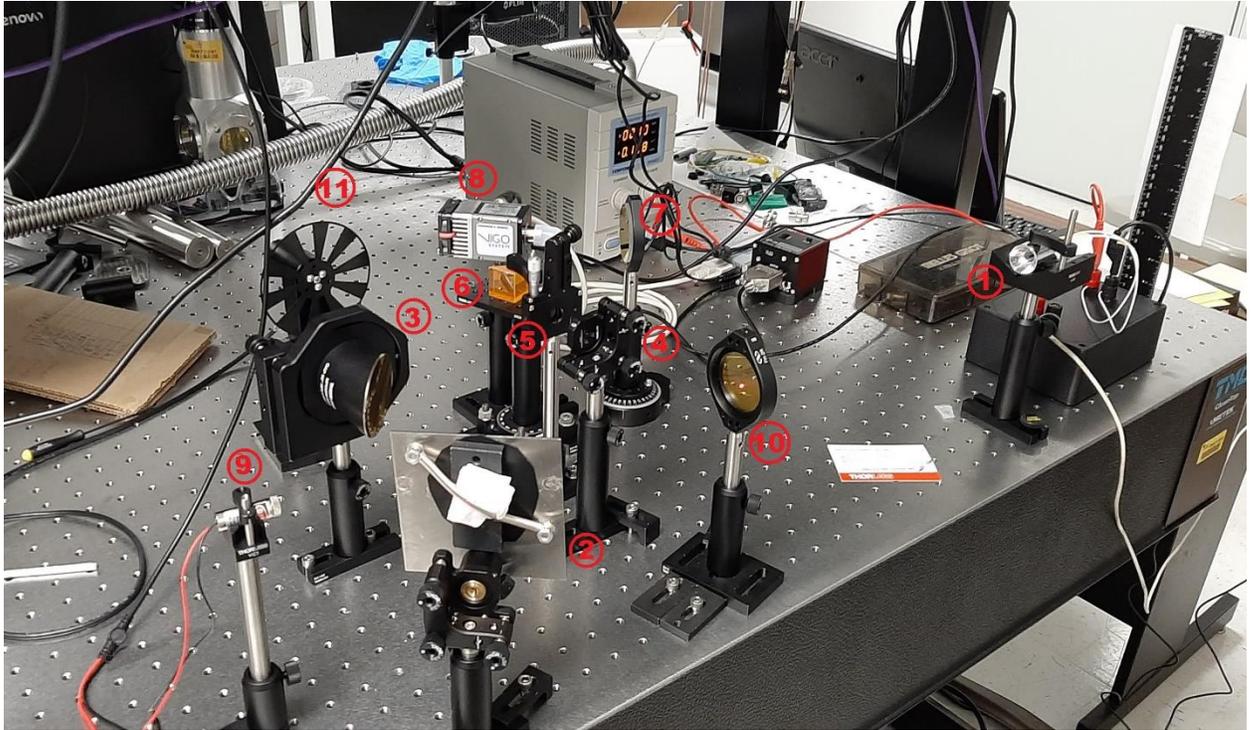


Figure 2. Layout of the miniaturized IR spectrometer system

Figure 2 is a photograph of the current configuration of the spectrometer in the Infrared Lab at NSTC. Annotations on the figure show the components of the spectrometer. A collimated infrared light source at (1) passes through an IR-transparent ZnSe window at (10) and projects broadband infrared energy towards the sample holder at (2). The sample holder is equipped with a mirror for alignment purposes. Energy reflected off the sample is gathered by an off-axis parabolic mirror at (3) which focuses the energy onto a smaller mirror at (4), concentrating the energy from a 25 mm beam to a 2 mm beam. This beam is further restricted by an adjustable slit at (5), then the narrow beam passes through the prism at (6), where it is spread in spectrum. This spread spectrum is scanned across the detector at (8) by the motorized rotating mirror at (7). Alignment is made difficult by the fact that the energy transported through the apparatus is invisible. To alleviate this problem, a visible red laser at (9) is reflected off the ZnSe window at (10) so as to be coaxial with the infrared light source's beam. The laser beam can then be aligned through the apparatus, aligning the path of the infrared energy as well. A chopper wheel, shown at (11), is going to be placed between the two off-axis parabolic mirrors, near their common focal points. This addition was necessary as the infrared energy reaching the detector is too small to be measurable. The signal modified by the chopper gives a 100 to 1000 times improvement in detection. With the use of a lock-in amplifier, the signal dispersed by the prism is now measurable.

The sample mount, labeled (2) in Figure 2, was replaced with a more stable custom-made stainless-steel plate to provide more repeatable positioning from sample to sample. The previous mount was simple to build and use but required too much re-alignment between samples.

In Year 1 a ZnSe prism with an apex angle of 8.5° was utilized since it allowed the red alignment laser beam to pass through the prism and trace the path all the way from source to detector. This prism provided a dispersion of wavelengths from 2-16 microns of only about 1° . It was found in practice that the signal at the detector is “blurred” by about the same amount. This is likely due to limited collimation of the light source and alignment inaccuracies in the apparatus. This situation required that we use a prism with a much larger apex angle of 45° . This prism yields a wavelength dispersion of about 10° , which should reduce signal blurring.

However, using this prism does not allow the red laser alignment beam to get past the prism as the index of refraction at $0.65\mu\text{m}$ (the wavelength of the laser) causes total internal reflection of the beam. The laser beam assists alignment up to its incidence on the face of the prism but is lost after that. Some other method of aligning the signal to the detector needs to be found. Alternatively, a prism with an intermediate angle, perhaps 30° , could be utilized, but these have not been found off-the-shelf in the marketplace. An alternate way to visualize the NIR laser source using external methods is being searched for.

Task 2: Sample Collection

- The team continues its partnership with UCF Recycles program in order to collect a statistically relevant plastic sample population.
- Most of the effort in this quarter has focused on improving the spectrometer design and operation, hence the effort in processing new samples has been reduced. New samples continue to be gathered but await processing until they are needed.
- Particularly since March, efforts of collecting new samples for library measurements have been challenging due to the ongoing COVID pandemic resulting in new restrictions and regulations. Focus has been diverted to optimize the optical setup and train the neural identification program.

Figure 3 shows a sampling of some soiled plastic samples that have been scanned into the plastic signature library. The FTIR MIR spectrometer focuses IR energy down to a small point and gathers the reflected energy. Of course, when the small spot focuses on a thick piece of contaminant, very little energy is reflected. However, when focused on a less severely soiled area, the generally unaffected plastic signature is reflected. The testbed spectrometer reflects IR energy over a broad area of the sample ($> 6\text{cm}^2$) and should be robust to sample contamination.



Figure 3. Examples of contaminated plastic samples.

Task 3: Optimization of the Identification Algorithm

- Neural networks trained on the sparse spectral data available in Year 1 gave encouraging results, but this year's effort will identify plastics based on the output of the test bench spectrometer. The first useable scans are anticipated to be produced in the second quarter of this year.
- The Center for Research in Computer Vision (CRCV) has been engaged to provide expert neural network development with the possible use of deep learning for plastic identification using this new data. This group has been provided with data from Year 1 so that they may become familiar with the project and they await the new scans to be provided next quarter.

Artificial intelligence based spectral fingerprint search:

In Year 1, the approach for automating classification with machine learning was to reduce the dimensionality of the input. The spectral signature produced by the spectrometer consists of 3271 data points of reflectance vs. wavenumber. As a first simple attempt at data reduction, we averaged the reflectance over 100 equally spaced consecutive wavelength intervals. Figure 4 displays the raw spectral signature of PVC, while Figure 5 shows the result of this wavelength averaging process on the PVC spectral signature. This process reduced the spectral resolution from 3271 data points to 100 points.

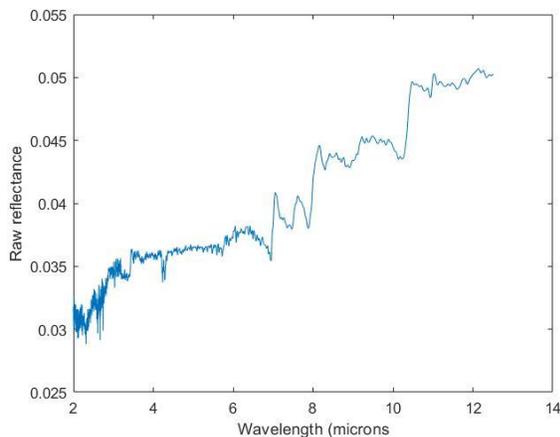


Figure 4. Raw spectrometer data (3271 points)

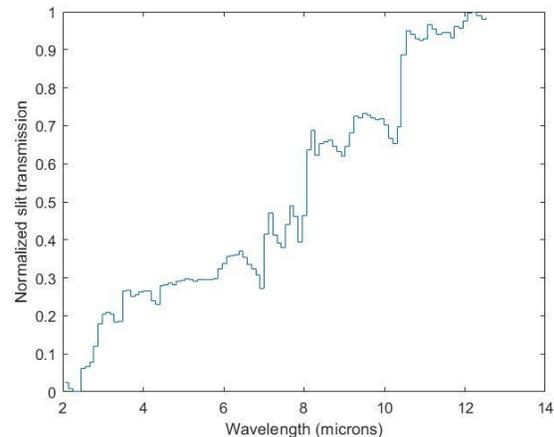


Figure 5. Wavelength average data (100 points)

This year, the simulated data will be replaced with actual scans produced by the spectrometer. It is anticipated that the scans will have significantly lower resolution than that shown in Figure 5 and will appear to be much “blurrier”. Perhaps the equivalent of a 20-point signature will be achieved.

Metrics:

1. List research publications resulting from **THIS** Hinkley Center project.
Ans: Under preparation.
2. List research presentations resulting from (or about) **THIS** Hinkley Center project.
Ans: The research has been presented as invited talks at University of Antioquia, Colombia in March and June, 2019.
3. List who has referenced or cited your publications from this project.
None
4. How have the research results from **THIS** Hinkley Center project been leveraged to secure additional research funding? What additional sources of funding are you seeking or have you sought?
Ans: We submitted the full proposal based on the preliminary work funded by Hinkley Center to EREF.
5. What new collaborations were initiated based on **THIS** Hinkley Center project?
Ans: Based on the same detection technique, we are helping University of Antioquia, Colombia to establish a coffee and avocado quality assessment process
6. How have the results from **THIS** Hinkley Center funded project been used (not will be used) by the FDEP or other stakeholders?

Ans: None to date.